





Lean In

COMPANY PROFILE

Daddy's Choice is committed to become one of the China Based Fortune 500 company. Established in 2015, Daddy's Choice is a high-tech enterprise that integrates the whole industrial chain of R&D, marketing, and distribution. After 5-years' high-speed development, Daddy's Choice has grown into a company with over 1000 employees, distribution channels and branches in more than 200 cities over 30 provinces, and 20000 plus retail outlets. Daddy's Choice always has international vision from the beginning of operation. It has been aggressively developing overseas market, setting up branches in the United States, Japan, Brazil, and etc.

Beijing Purism Technology Co., Ltd., founded on March 21, 2019, is a high-tech enterprise dedicated to research, development and production of personal care products and protective equipment. We aim to create a purist way of life with extreme efforts to benefit the world.



CORPORATE R&D CAPABILITIES

JAPAN LABORATORY

As Daddy's Choice's overseas laboratory, Japanese laboratory integrated global cutting-edge scientific and technological achievements in an open manner, recruited high-tech talents, and started a special cooperation with prof, Fujino Hideaki, a renowned medical doctor and doctoral supervisor at Kobe University in Japan. Research areas include shampoos, shower gels, animal skin irritation tests and patent license.

BEIJING LABORATORY

As Daddy's Choice's headquarters for R&D in china, Beijing laboratory has taken the lead in combining new product development with consumer surveys. It has received thousands of people including leaders from all walks of life, maternal and child , medical, health, media and consumer groups. It is praised as a research and development vane of the industry.



GLOBAL SUPPLY

The global delivery of Purism series of protective equipment is available in the United States, Brazil, France, Germany, Egypt, Russia, Japan, Australia and other countries. The logistics system is strong, fast and reliable.



PRODUCTION BASE DEZHOU, SHANDONG

At the end of January 2020, Purism set up the production line project team of protective materials (face masks / protective clothing), and started to build the whole industrial chain of upstream raw materials, middle end factory manufacturing and end online and offline sales of "Purism" brand masks. To produce high quality personal protective products according to international standards.





立体1号

PRODUCTION BASE CHUZHOU, ANHUI

At present, the two major factories (Linyi, Shandong / Chuzhou, Anhui) have been put into operation stably, with a total plant area of over 150000 square meters, and 65 production lines have been put into operation. They produce FFP2 & FFP3 masks, disposable medical masks, medical surgical masks, protective clothing and other protective products, with a daily production capacity of nearly 2.8 million. In addition, there are 12 melt blown cloth raw material production lines.



立体2号



立体3号

立体4号

立体5号

立体6号

立体7号

立体8号

立体9号

立体10号


立体11号

立体12号

AUTHENTICATION –FFP2 T0001



CE MODULE B

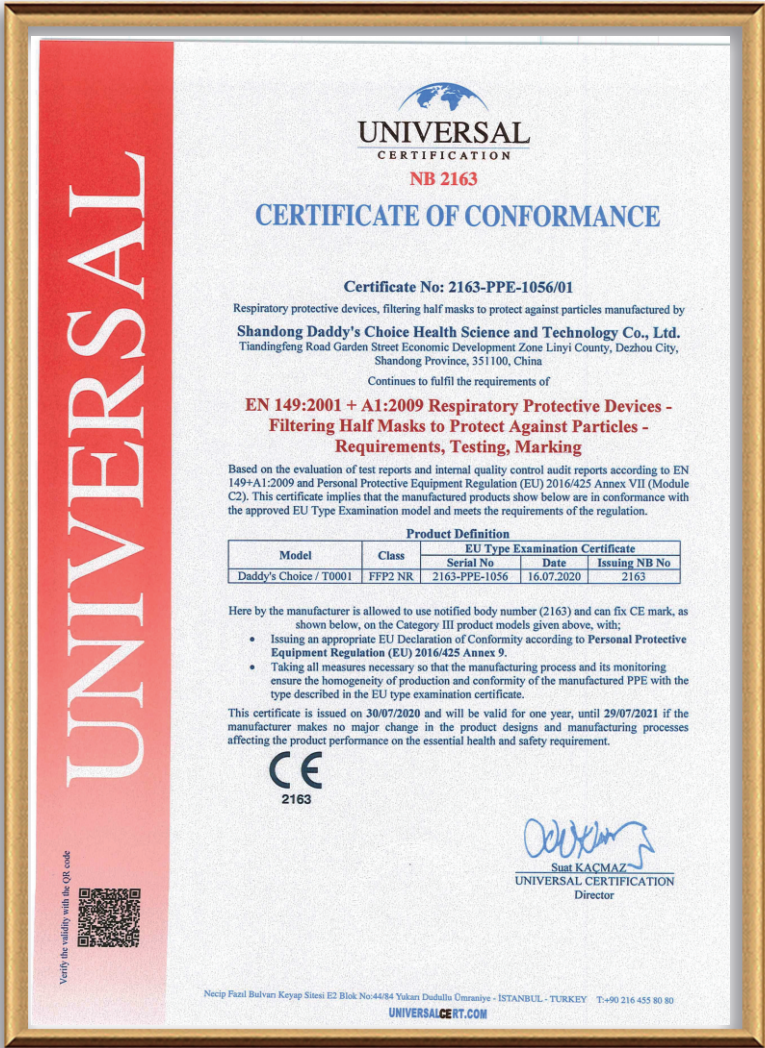

CE MODULE C

FFP2 T0001 FILTERING HALF MASK

- Non woven fabric
- Meltblown nonwoven



AUTHENTICATION – FFP2 PURISM



SGS CE



SGS CE

FFP2 PURISM PROTECTIVE FACE MASK

- Non woven fabric
- Meltblown nonwoven



PARTICULATE RESPIRATOR FFP3

LGAI Technological Center, S.A. (APPLUS)
Campus UAB - Ronda de la Font del Carme s/n
08193 Bellaterra (Barcelona)
T +34 93 557 20 00
www.applus.com

Applus⁺

CERTIFICADO DE EXAMEN UE DE TIPO
EU-TYPE EXAMINATION CERTIFICATE

CE Notified Body No. 0370

ENAC CERTIFICACIÓN N° 1210-PR-04

No. **0370-4154-PPE/B**

ORGANISMO NOTIFICADO N° <i>NOTIFIED BODY NUMBER</i>	0370 - LGAI TECHNOLOGICAL CENTER (APPLUS)
SOLICITANTE <i>APPLICANT</i>	Shandong Daddy's Choice Health Science and Technology Co., Ltd. Tiandingfeng road, Garden street, Economic Development Zone, Linyi County, Dezhou City, Shandong Province
FABRICANTE <i>MANUFACTURER</i>	Shandong Daddy's Choice Health Science and Technology Co., Ltd. Tiandingfeng road, Garden street, Economic Development Zone, Linyi County, Dezhou City, Shandong Province
REGLAMENTO DE APLICACIÓN PARA DAR LA CONFORMIDAD / APPLICABLE REGULATION TO GIVE CONFORMITY: REGLAMENTO (UE) 2016/425 SOBRE LOS EQUIPOS DE PROTECCIÓN INDIVIDUAL REGULATION (EU) 2016/425 PERSONAL PROTECTIVE EQUIPMENT	
PROCEDIMIENTO DE EVALUACIÓN DE LA CONFORMIDAD <i>CONFORMITY ASSESSMENT PROCEDURE</i>	Módulo II / Module: B EXAMEN UE DE TIPO / EU TYPE EXAMINATION
IDENTIFICACIÓN DEL EPI (NÚMERO DE TIPO) <i>IDENTIFICATION OF THE PPE (TYPE NUMBER)</i>	Ref.: C001 Particulate Respirator
NIVEL O NIVELES DE RENDIMIENTO O LA CLASE DE PROTECCIÓN DEL EPI / PERFORMANCE LEVEL OR PROTECTION CLASS OF THE PPE	FFP3 NR
NORMAS ARMONIZADAS / HARMONISED STANDARDS	EN 149:2001 + A1:2009 Dispositivos de protección respiratoria. Medias máscaras filtrantes de protección contra partículas. Requisitos, ensayos, marcado. <i>EN 149:2001 + A1:2009 Respiratory protective devices. Filtering half masks to protect against particles. Requirements, testing, marking</i>
FECHA DE EMISIÓN / ISSUE DATE	05/08/2020
VALIDEZ HASTA / VALIDITY UNTIL	05/08/2025

El presente certificado se mantendrá vigente durante 5 años siempre que el producto descrito no sea modificado y cumpla los requisitos esenciales de salud y seguridad establecidos en el Reglamento (UE) 2016/425. Para asegurar dicho cumplimiento, este certificado deberá ir acompañado de la documentación correspondiente a la Evaluación de Conformidad con el tipo según módulo C2, D (realizada por un Organismo Notificado, según frecuencia establecida).

This certificate will remain valid for 5 years as long as the indicated product is not modified and fulfils the essential requirements of health and safety established in (EU) Regulation 2016/425. To ensure such compliance, this certificate must be accompanied by the documentation corresponding to the Conformity Assessment to type according to C2, D (carried out by a Notified Body according to the established frequency).

Applus⁺
Xavier Ruiz Peña
Managing Director, Product Conformity B.U.

Este documento carece de validez sin su anexo técnico, cuyo número coincide con el del certificado.
This document is not valid without its technical annex, whose number coincides with the number of certificate.

Puede comprobarse la validez de este certificado en nuestra página web / You can check the validity of this certificate into our website at:
www.appluslaboratories.com/certified_products

Page 1 of 2

LGAI TECHNOLOGICAL CENTER, S.A. CIF: A-63207492



FFP3 CE Certification Module B issued by Applus(NB 0370)

PARTICULATE RESPIRATOR FFP2

LGAi Technological Center, S.A. (APPLUS)
Campus UAB - Ronda de la Font del Carme s/n
08193 Bellaterra (Barcelona)
T +34 93 567 20 00
www.applus.com

Applus⁺

CERTIFICADO DE EXAMEN UE DE TIPO
EU-TYPE EXAMINATION CERTIFICATE

CE **ENAC** No. **0370-4223-PPE/B**

ORGANISMO NOTIFICADO Nº <i>NOTIFIED BODY NUMBER</i>	0370 - LGAI TECHNOLOGICAL CENTER (APPLUS)
SOLICITANTE <i>APPLICANT</i>	Shandong Daddy's Choice Health Science and Technology Co.,Ltd. Tiandingfeng road Garden street Economic Development Zone Linyi County Dezhou City Shandong Province
FABRICANTE <i>MANUFACTURER</i>	Shandong Daddy's Choice Health Science and Technology Co.,Ltd. Tiandingfeng road Garden street Economic Development Zone Linyi County Dezhou City Shandong Province

REGLAMENTO DE APLICACIÓN PARA DAR LA CONFORMIDAD / APPLICABLE REGULATION TO GIVE CONFORMITY:
REGLAMENTO (UE) 2016/425 SOBRE LOS EQUIPOS DE PROTECCIÓN INDIVIDUAL
REGULATION (EU) 2016/425 PERSONAL PROTECTIVE EQUIPMENT

PROCEDIMIENTO DE EVALUACIÓN DE LA CONFORMIDAD <i>CONFORMITY ASSESSMENT PROCEDURE</i>	Módulo II / Module: B EXAMEN UE DE TIPO / EU TYPE EXAMINATION
IDENTIFICACIÓN DEL EPI (NÚMERO DE TIPO) <i>IDENTIFICATION OF THE PPE (TYPE NUMBER)</i>	Ref.: C002 Particulate Respirator
NIVEL O NIVELES DE RENDIMIENTO O LA CLASE DE PROTECCIÓN DEL EPI / PERFORMANCE LEVEL OR PROTECTION CLASS OF THE PPE	FFP2 NR
NORMAS ARMONIZADAS / HARMONISED STANDARDS	EN 149:2001 + A1:2009 Dispositivos de protección respiratoria. Medias máscaras filtrantes de protección contra partículas. Requisitos, ensayos, marcado. <i>EN 149:2001 + A1:2009 Respiratory protective devices. Filtering half masks to protect against particles. Requirements, testing, marking</i>
FECHA DE EMISIÓN / ISSUE DATE	19/08/2020
VALIDEZ HASTA / VALIDITY UNTIL	19/08/2025

El presente certificado se mantendrá vigente durante 5 años siempre que el producto descrito no sea modificado y cumpla los requisitos esenciales de salud y seguridad establecidos en el Reglamento (UE) 2016/425. Para asegurar dicho cumplimiento, este certificado deberá ir acompañado de la documentación correspondiente a la Evaluación de Conformidad con el tipo según módulo C2, D (realizada por un Organismo Notificado, según frecuencia establecida).

This certificate will remain valid for 5 years as long as the indicated product is not modified and fulfills the essential requirements of health and safety established in (EU) Regulation 2016/425. To ensure such compliance, this certificate must be accompanied by the documentation corresponding to the Conformity Assessment to type according to C2, D (carried out by a Notified Body according to the established frequency).

Applus⁺
LGAi Technological Center, S.A.
Xavier Ruiz Peña
Managing Director, Product Conformity B.U.



Este documento carece de validez sin su anexo técnico, cuyo número coincide con el del certificado.
This document is not valid without its technical annex, whose number coincides with the number of certificate.
Puede comprobarse la validez de este certificado en nuestra página web / You can check the validity of this certificate into our website at:
www.appluslaboratorios.com/certified_products

Page 1 of 2



FFP2 CE Certification Module B issued by Applus(NB 0370)

AUTHENTICATION – DISPOSABLE SURGICAL MASK



中国认可
国际互认
检测
TESTING
CNAS L0599



Test Report SL52025258709901TX Date: June 17, 2020
CHUZHOU DADDY'S CHOICE SCIENCE AND TECHNOLOGY CO., LTD
MIDDLE OF NANJING ROAD, LANGYA DISTRICT, CHUZHOU CITY, ANHUI PROVINCE.

Page 1 of 3

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Surgical mask
Composition : (A)66% Non-woven fabric, 34% melt-blown fabric
Sample Color : (A)Blue and White
Manufacturer : CHUZHOU DADDY'S CHOICE SCIENCE AND TECHNOLOGY CO., LTD
Lot No. : 20200524
Proposed Care Instruction : -
Test Performed : Selected test(s) as requested by applicant
Sample Receiving Date : May 26, 2020
Testing Period : May 26, 2020 - Jun 17, 2020
Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center



Sara Guo (Account Executive) Helen Xuan (Authorized Signatory)

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/terms-and-conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and arbitration clauses defined therein. Any holder of this document is advised that information on the Company's data the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not constitute parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: CH.Overseas@sgs.com

1/ Building No. 388, Yamen Road, Kailash District, Shanghai, China 200233 1 (86-21) 61420966 1 (86-21) 64692763 www.sgsnsp.com.cn
2/ Building No. 388, Yamen Road, Kailash District, Shanghai, China 200233 1 (86-21) 61420966 1 (86-21) 64692763 e.sgs.china@sgs.com

中国·上海·徐汇区宜山路388号3号楼 邮编: 200233 1 (86-21) 61420966 1 (86-21) 64692763

Member of the SGS Group (SGS SA)

SGS Test Report



Test Report SL52025258709901TX Date: June 17, 2020 Page 2 of 3

Test Result

Standard Specification for Performance of Materials Used in Medical Face Masks
(ASTM F2100-2019)

Section 6.1 Bacterial filtration efficiency (BFE)
(ASTM F2101)

	1#	2#	3#	4#	5#
(BFE), %	99.4	99.7	99.8	99.7	99.7

Remark: Performance Requirement: Level 1 $\geq 95\%$, Level 2 $\geq 98\%$, Level 3 $\geq 98\%$

Section 6.1 Differential Pressure
(EN 14683 :2019 Annex C, Flow rate 8 l/min)

	1#	2#	3#	4#	5#
Differential pressure ΔP (mm H ₂ O/cm ²)	2.4	2.7	2.8	3.1	2.9

Remark: Performance Level: Level 1 Barrier: $<5.0\text{mm H}_2\text{O/cm}^2$, Level 2 Barrier: $<6.0\text{mm H}_2\text{O/cm}^2$, Level 3 Barrier: $<6.0\text{mm H}_2\text{O/cm}^2$

Section 6.1 Resistance to Penetration by Synthetic Blood
(ASTM F1862/F1862M-2017)

Pressure 160mmHg

Penetration on inside surface

1#	2#	3#	4#	5#	6#	7#	8#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass
9#	10#	11#	12#	13#	14#	15#	16#
Pass	Pass	Pass	Fail	Pass	Pass	Pass	Pass
17#	18#	19#	20#	21#	22#	23#	24#
Pass	Pass	Pass	Pass	Pass	Pass	Fail	Pass
25#	26#	27#	28#	29#	30#	31#	32#
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass

Number of Pass: 30
Overall result: Acceptable

Remark:

- 1) Performance Requirement Level 1 Barrier: 80mmHg, Level 2 Barrier: 120mmHg, Level 3 Barrier: 160mmHg
- 2) Distance of the medical face mask target area surface to the tip of cannula is 30.5cm.
- 3) Condition and Test temperature (21 \pm 5)°C, relative humidity (85 \pm 5)%
- 4) An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show pass results

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/terms-and-conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/terms-and-conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and arbitration clauses defined therein. Any holder of this document is advised that information on the Company's data the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not constitute parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing inspection report & certificate, please contact us at telephone: (86-755) 8387 1443, or email: CH.Overseas@sgs.com

1/ Building No. 388, Yamen Road, Kailash District, Shanghai, China 200233 1 (86-21) 61420966 1 (86-21) 64692763 www.sgsnsp.com.cn
2/ Building No. 388, Yamen Road, Kailash District, Shanghai, China 200233 1 (86-21) 61420966 1 (86-21) 64692763 e.sgs.china@sgs.com

中国·上海·徐汇区宜山路388号3号楼 邮编: 200233 1 (86-21) 61420966 1 (86-21) 64692763

Member of the SGS Group (SGS SA)


SGS Test Report

DISPOSABLE SURGICAL MASK


EN 14683 Type IIR

3 Ply Protection


- Leak Proof Non-Woven Fabric(New Non-woven Fabric)
- Effectively Inhibit and Isolate Harmful Particles and Gases
- High Density Filter Layer(Fine Melt-blown Non-woven Fabric)
- Great Efficient at Filtering out Fine Particles
- Direct Contact Skin Layer(New Non-woven Fabric)
- Moisture-proof, Breathable, Non-toxic, Non-stimulating, Soft and Skin-friendly

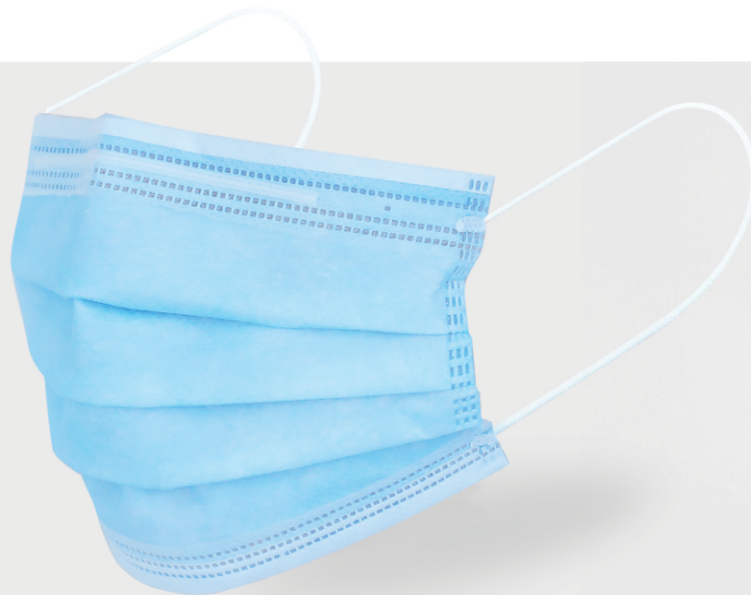

AUTHENTICATION – DISPOSABLE MEDICAL MASK

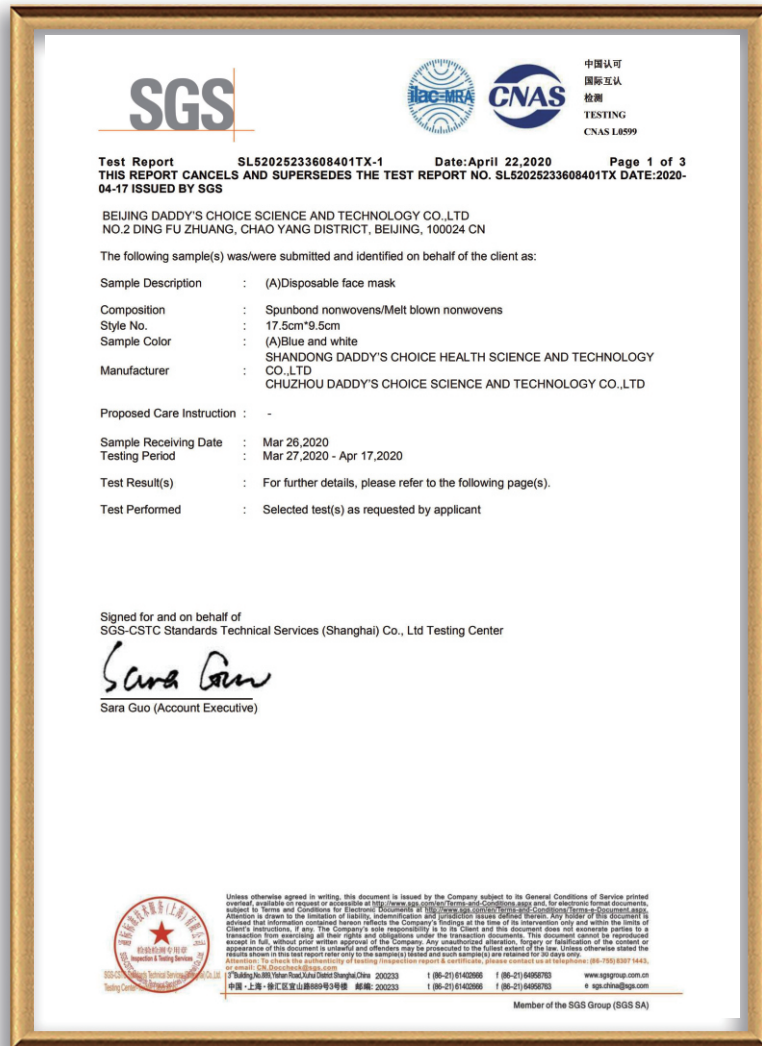

SGS Test Report EN 14683:2019

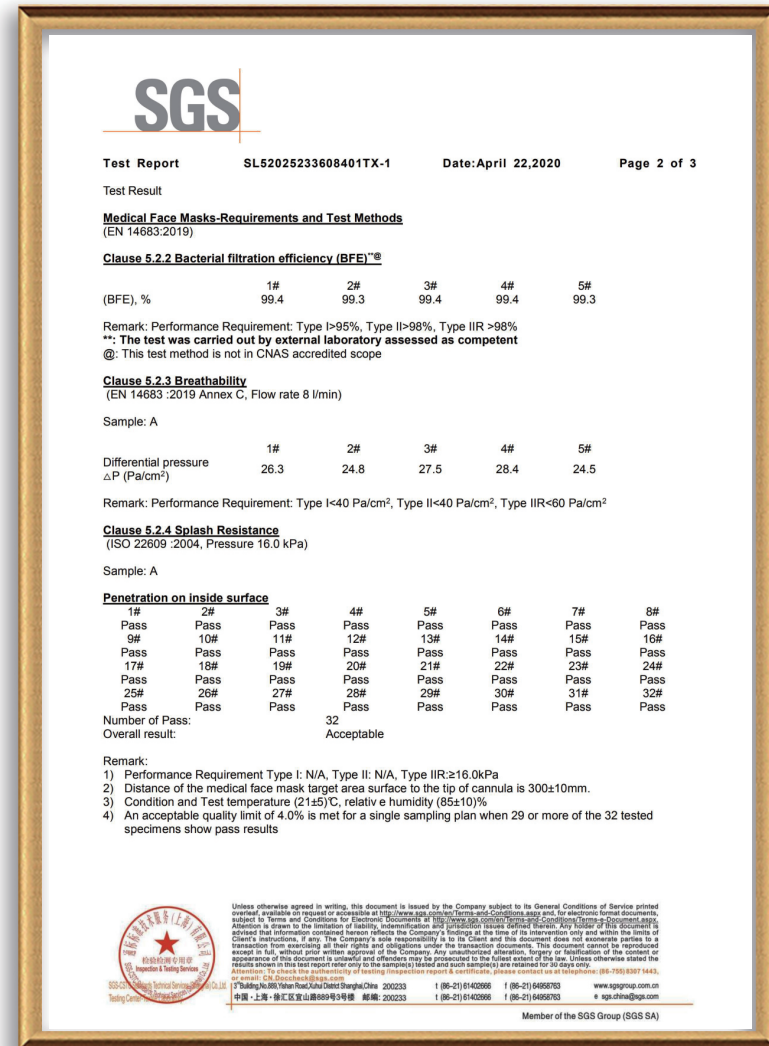

SGS Test Report EN 14683:2019

DISPOSABLE MEDICAL MASK

EN 14683 Type I



MELTBLOWN



DETECTION



MULTI-LAYER



SKIN-FRIENDLY



BREATHABLE



COMFORTABLE TO WEAR



AUTHENTICATION – NITRILE GLOVE

SGS

Test Report

No.: QDHL2007007319MD Date: AUG.10,2020 Page 1 of 4

SHANDONG DADDY'S CHOICE HEALTH SCIENCE AND TECHNOLOGY CO.,LTD.
TIANDINGFENG ROAD GARDEN STREET ECONOMIC DEVELOPMENT
ZONE LINYI COUNTY DEZHOU CITY SHANDONG PROVINCE

The following sample(s) was/were submitted and identified by the client as:
Sample Description : MEDICAL EXAMINATION GLOVES
Lot No. : NOT PROVIDED
Lot Size : NOT PROVIDED
Sample Quantity : 500PCS
Style/ Item No. : G001
Sample Receiving Date : JUL.24,2020
Testing Period : JUL.24,2020 TO AUG.10,2020

Test Requested

Result

BS EN 455-1:2000 Medical Gloves for Single Use – Part 1: Requirements and Testing for Freedom from Holes (Clause 5.1)

Pass

BS EN 455-2:2015 Medical Gloves for Single Use – Part 2: Requirements and Testing for Physical Properties (Clause 4.2, 4.3, 5.2, 5.3.)

Pass

Note: -Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.

SGS-CSTC Standards
Technical Services (Qingdao)
Co., Ltd.

Jessica Gao

SGS

QDHL2007007319MD

Jessica Gao

Approved Signatory

Member of the SGS Group (SGS SA)

SGS EN455-1 EN455-2 Test Report

SGS

Test Report

No.: QDHL2007007319MD Date: AUG.10,2020 Page 2 of 4

Test Results :
BS EN 455-1:2000 Medical gloves for single use – Part 1: Requirements and testing for freedom from holes

Number of test sample

:

200 PCS

Sample size

:

L

Number of non-conforming gloves

:

1 PC

Clause

Test Items

Result

5

Watertightness test for detection of holes

5.1

Referee testing

Pass (See note 1)

Note

:

1

Sample quantity: 200pcs, AQL:1.5, Ac:7, Re:8, Found:1 Pc.
The sample selecting amount for this clause is deviated to 200 pcs as assessed by SGS.

BS EN 455-2:2015 Medical gloves for single use – Part 2: Requirements and testing for physical properties

Number of test sample

:

26 PCS

Type

:

Examination/procedure gloves b)

Size

:

Examination/procedure gloves: L

Clause

Test Items

Result

4

Dimensions

4.2

Length

Pass (See result 1)

4.3

Width

Pass (See result 1)

5

Strength

5.2

Force at break

Pass (See result 2)

5.3

Force at break after challenge testing

Pass (See result 2)

Member of the SGS Group (SGS SA)

SGS EN455-1 EN455-2 Test Report

NITRILE GLOVE

High Elasticity

Ultrathin

Super Fit



DISPOSABLE PROTECTIVE COVERALL

- ✓ Good barrier
- ✓ Hot air adhesive strip
- ✓ Technical requirements for disposable protective clothing for medical use



DIAPER & PERSONAL CARE


"Daddy's Choice" redefines China's mother and baby products. It's the first new national baby care brand with a concept of "Safe and Clean Without Additions". There is no fragrance, pigment, formaldehyde, fluorescent agent and other harmful additives, which brings consumers the most extreme product experience with ultimate performance.



QUALITY CONTROL SYSTEM

Technical advantages

The company has established a sound quality system in accordance with the "medical device production quality management specifications" 《医疗器械生产质量管理规范》, and maintained effective operation. The production plant, equipment, human resources and other resources meet the production requirements of products, and the control of procurement, production process, inspection and other links is complete and effective.

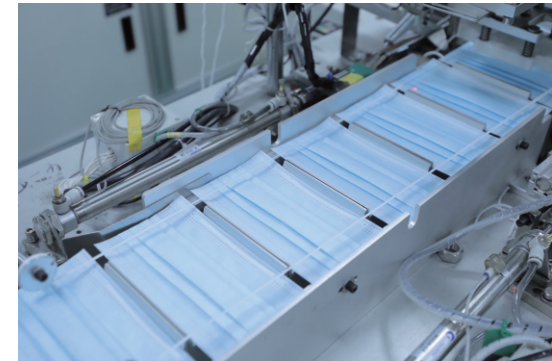

process control

Our company has a 100000 level sterile medical equipment production workshop of more than 500 square meters, equipped with a full-automatic mask production line. More than 100 square meters of 10000 level microbial testing laboratory is equipped with biosafety cabinet, super clean bench, vertical steam sterilization pot and other microbial testing equipment. The physical research and development laboratory is more than 100 square meters, equipped with testing and development equipment such as mask filtration performance tester, synthetic blood penetrant tester, mask bacterial filtration efficiency tester, tightness tester, etc., with complete research and development, production and testing capabilities of medical surgical masks and medical protective masks.






Equipment test

The comprehensive performance indexes of our company's sterile medical device production workshop and microbiological testing laboratory all meet the requirements of the level control of cleanliness (static) in the clean room (Interior) specified in the appendix of "quality management specification for medical device production sterile medical device".



Germany:

Yiwu-Hamburg GmbH
Baumgartenstrasse 14a,
26122 Oldenburg
HRB 215505 AG Oldenburg

 www.daddys-choice.de
 axelstoyke@daddys-choice.de
 +49 173 5276974 (Germany)
+86 180 72326669 (China)

China:

Shandong Daddy's Choice Health Science and Technology Co., Ltd.
Tiandingfeng road Garden street Economic Development Zone Linyi County
Dezhou City Shandong Province 251500 CN.

ChuZhou Daddy's Choice Science and Technology Co.,Ltd.
Middle of Nanjing Road,Langya District,Chuzhou City,Anhui Province.